

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281 LW Holland

08/24/11

Test No: 416296


Animal and Sample Description

Animal Name: AH Peruvian Casanova
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Grey

Animal ID: 528210000241099
Sample Location: Side
Sample Date: 04/21/11
Age: 02/05/03

Laboratory Data

Mean Fiber Diameter: 24.8 microns
Standard Deviation: 5.9 microns
Coefficient of Variation: 23.6 %
Fibers Greater Than 30 microns: 12.3 %

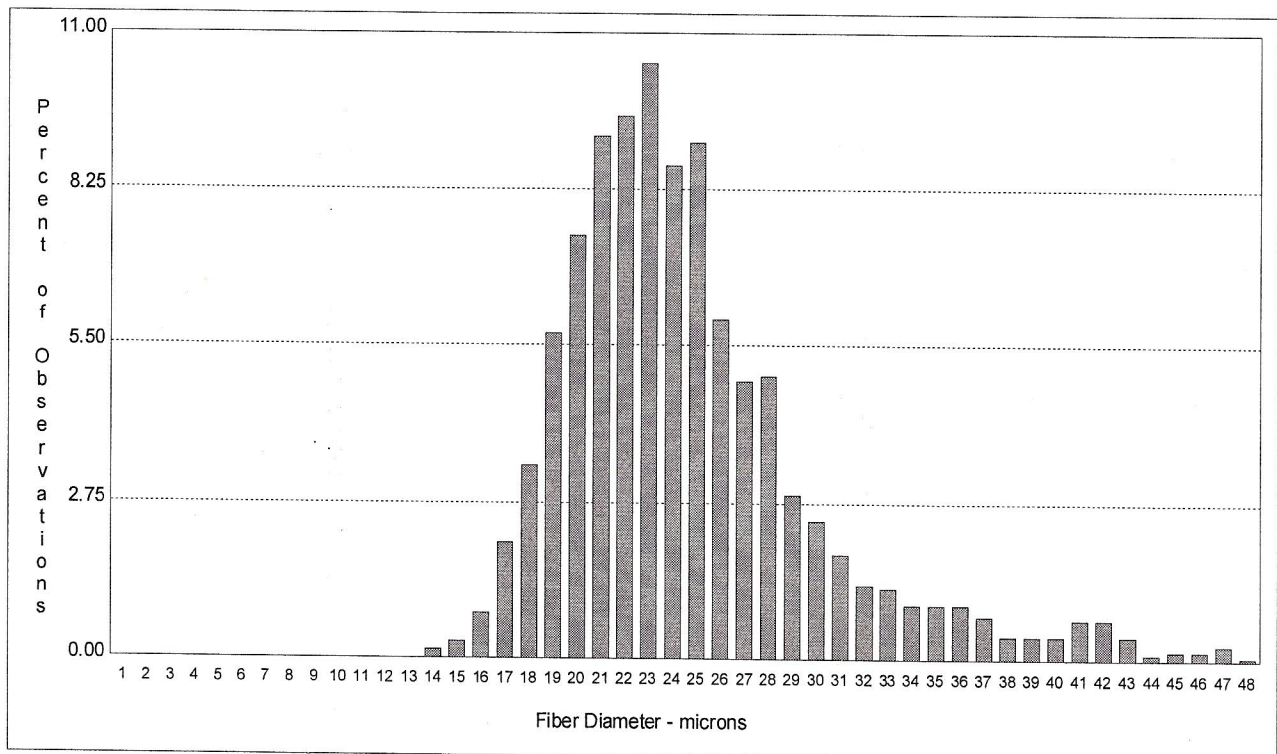

This Test Performed According to I.W.T.O Method 12