

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281LW Netherlands

07/28/12

Test No: 436934


Animal and Sample Description

Animal Name: AH Peruvian Charlene
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 0006E8D871
Sample Location: Side
Sample Date: 05/02/12
Age: 06/30/11

Laboratory Data

Mean Fiber Diameter:	19.8 microns	Spin Fineness:	18.7 microns
Standard Deviation:	3.5 microns	Mean Curvature (deg/mm):	47.6
Coefficient of Variation:	17.4 %	SD Curvature (deg/mm):	25.6
Fibers Greater Than 30 microns:	0.8 %	Comfort Factor:	99.2 %
Medullated Fibers:	1.3 %		

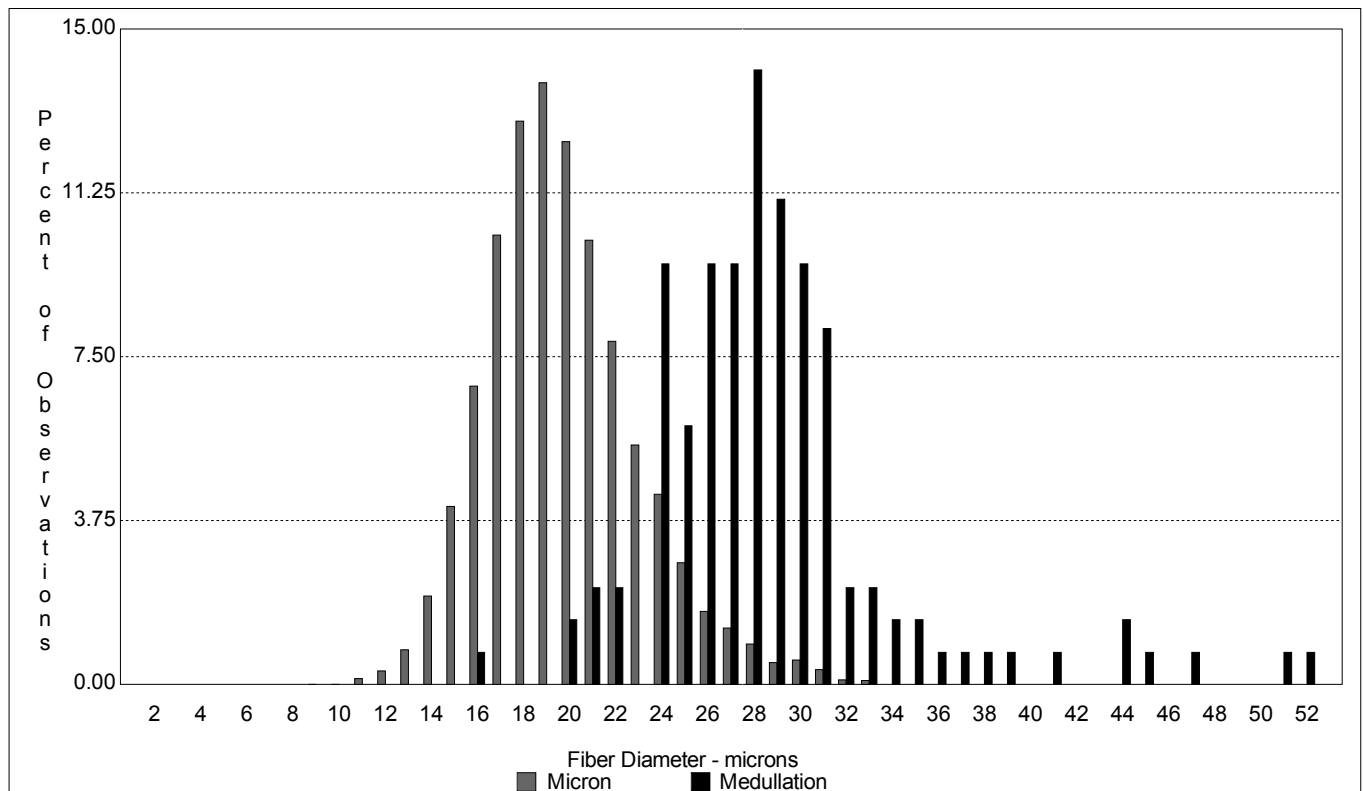

This Test Performed According to I.W.T.O Method 47