



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281LW Netherlands

Date: 06/03/1

Test No: 47766


Animal and Sample Description

Animal Name: AH Peruvian Christiano
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 0006E8ED4B
Sample Location: Side
Sample Date: 04/23/14
Age: 06/21/09

Laboratory Data

Mean Fiber Diameter:	20.7 microns	Fibers Greater Than 30 microns:	3.6 %
Standard Deviation:	4.4 microns	Comfort Factor:	96.4 %
Coefficient of Variation:	21.1 %	Mean Curvature:	39.1 deg/mm
Spin Fineness:	20.1 microns	SD Curvature:	23.1 deg/mm

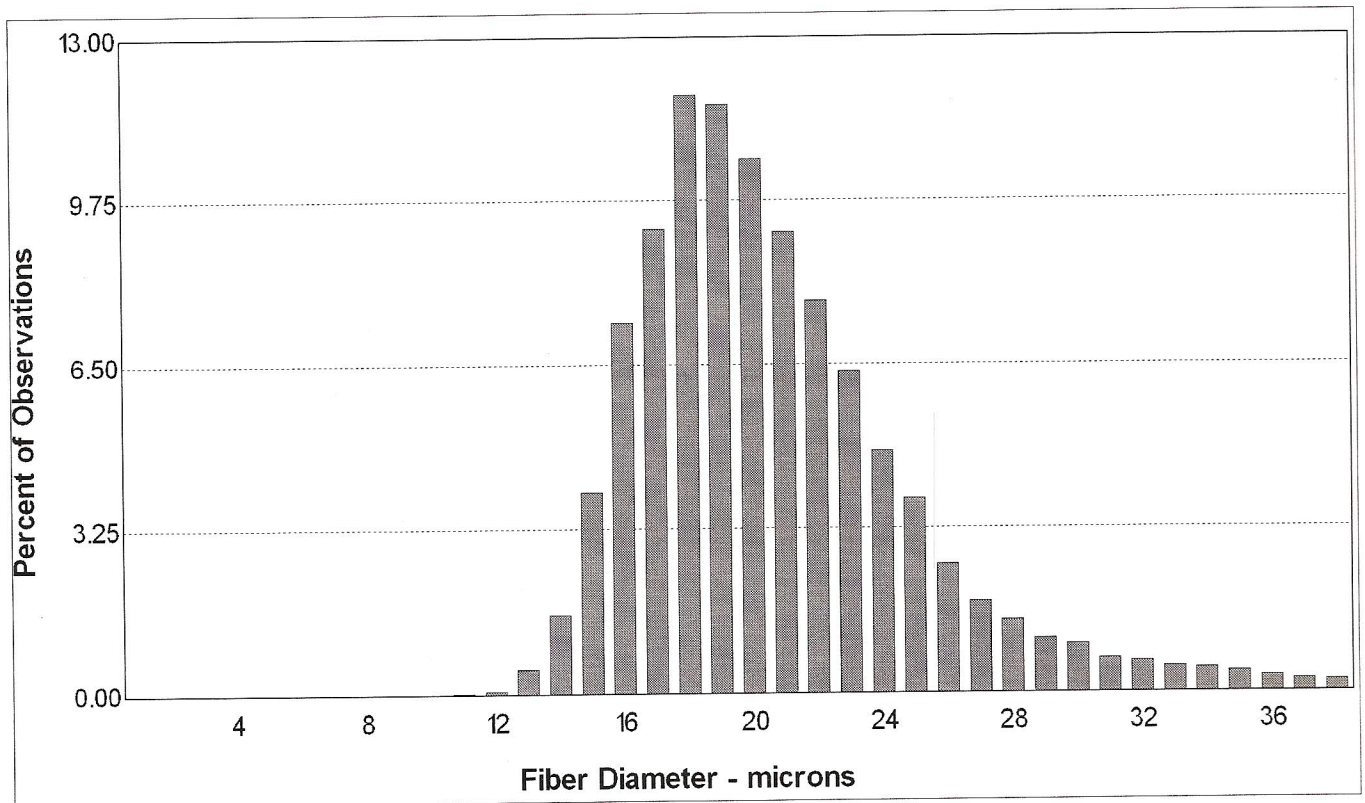

This Test Performed According to I.W.T.O Method 47