

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281LW Netherlands

Date: 05/14/15

Test No: 500947


Animal and Sample Description

Animal Name: AH Peruvian Christiano
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 6E8ED4B
Sample Location: Side
Sample Date: 04/17/15
Age: 06/21/09

Laboratory Data

Mean Fiber Diameter:	21.6 microns	Fibers Greater Than 30 microns:	5.4 %
Standard Deviation:	4.8 microns	Comfort Factor:	94.6 %
Coefficient of Variation:	22.0 %	Mean Curvature:	40.8 deg/mm
Spin Fineness:	21.2 microns	SD Curvature:	21.0 deg/mm

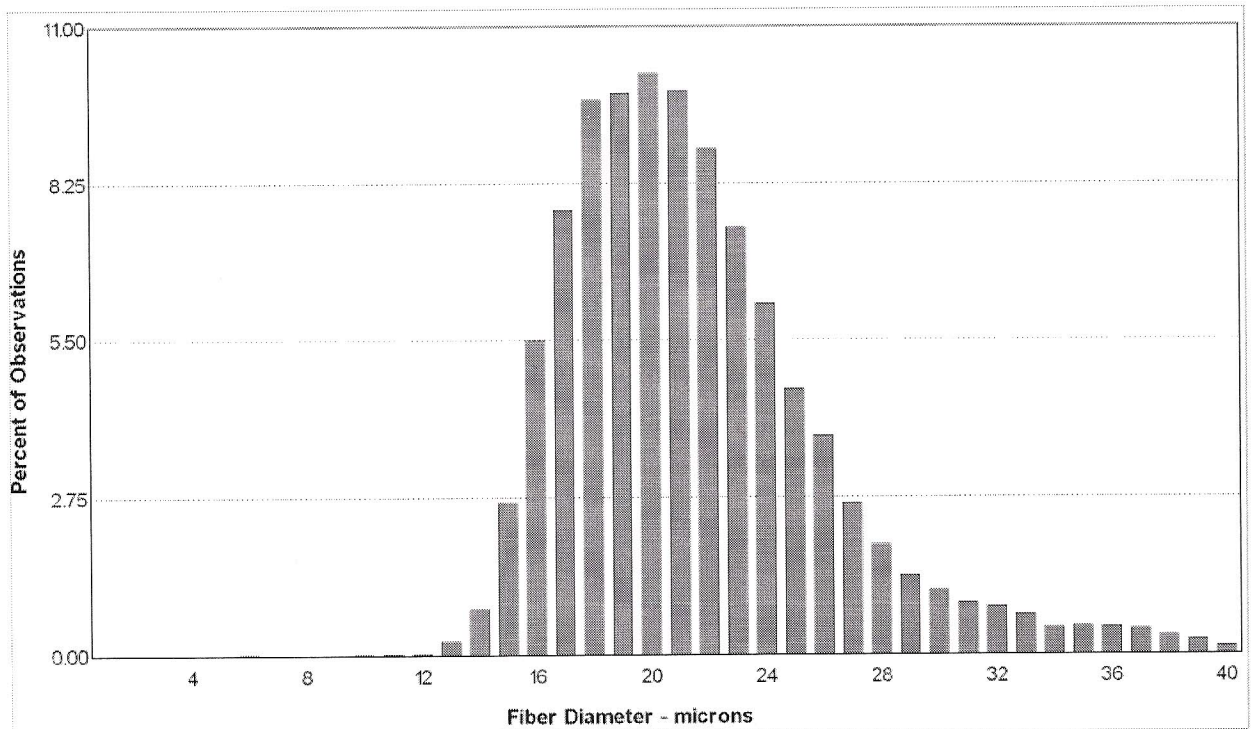

This Test Performed According to I.W.T.O Method 47