



Yocom-McColl Testing Laboratories, Inc.
 540 West Elk Place • Denver, Colorado 80216-1823 USA
 PHONE (303) 294-0582 • FAX (303) 295-6944
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
 Micron Test Report**

Alpaca Holland/Jan van den Hoek
 Rijksstraatweg 94
 Numansdorp 3281LW Netherlands

07/28/12

Test No: 436948


Animal and Sample Description

Animal Name: AH Peruvian Christiano
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 0006E8ED4B
Sample Location: Side
Sample Date: 05/02/12
Age: 06/21/09

Laboratory Data

Mean Fiber Diameter:	21.1 microns	Spin Fineness:	20.4 microns
Standard Deviation:	4.3 microns	Mean Curvature (deg/mm):	45.2
Coefficient of Variation:	20.3 %	SD Curvature (deg/mm):	27.9
Fibers Greater Than 30 microns:	3.6 %	Comfort Factor:	96.4 %
Medullated Fibers:	15.2 %		

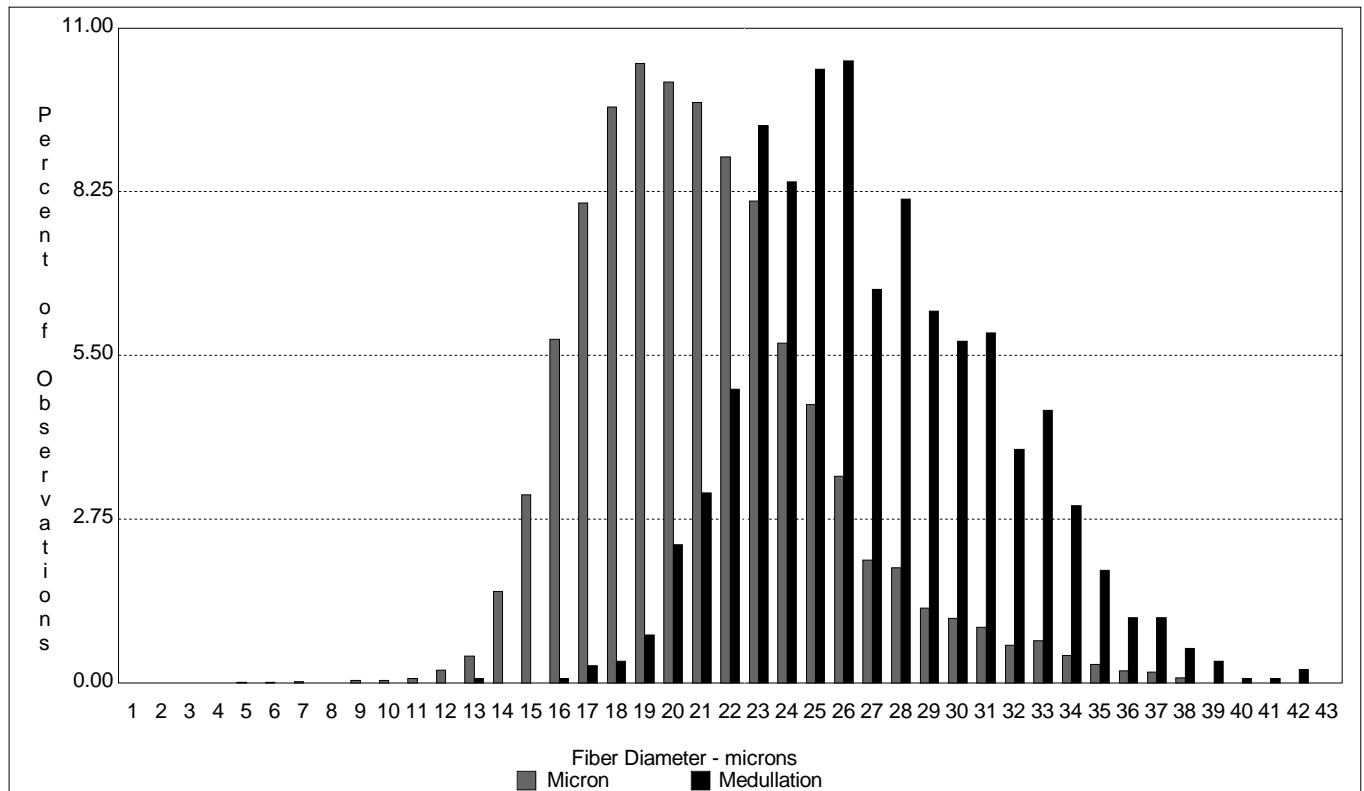

This Test Performed According to I.W.T.O Method 47