



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281LW Netherlands

Date: 03/25/14

Test No: 475451


Animal and Sample Description

Animal Name: AH Peruvian Julian
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 006E8A956
Sample Location: Side
Sample Date: 03/17/14
Age: 07/07/11

Laboratory Data

Mean Fiber Diameter:	18.8 microns	Fibers Greater Than 30 microns:	0.3 %
Standard Deviation:	2.8 microns	Comfort Factor:	99.7 %
Coefficient of Variation:	14.8 %	Mean Curvature:	39.9 deg/mm
Spin Fineness:	17.4 microns	SD Curvature:	21.9 deg/mm

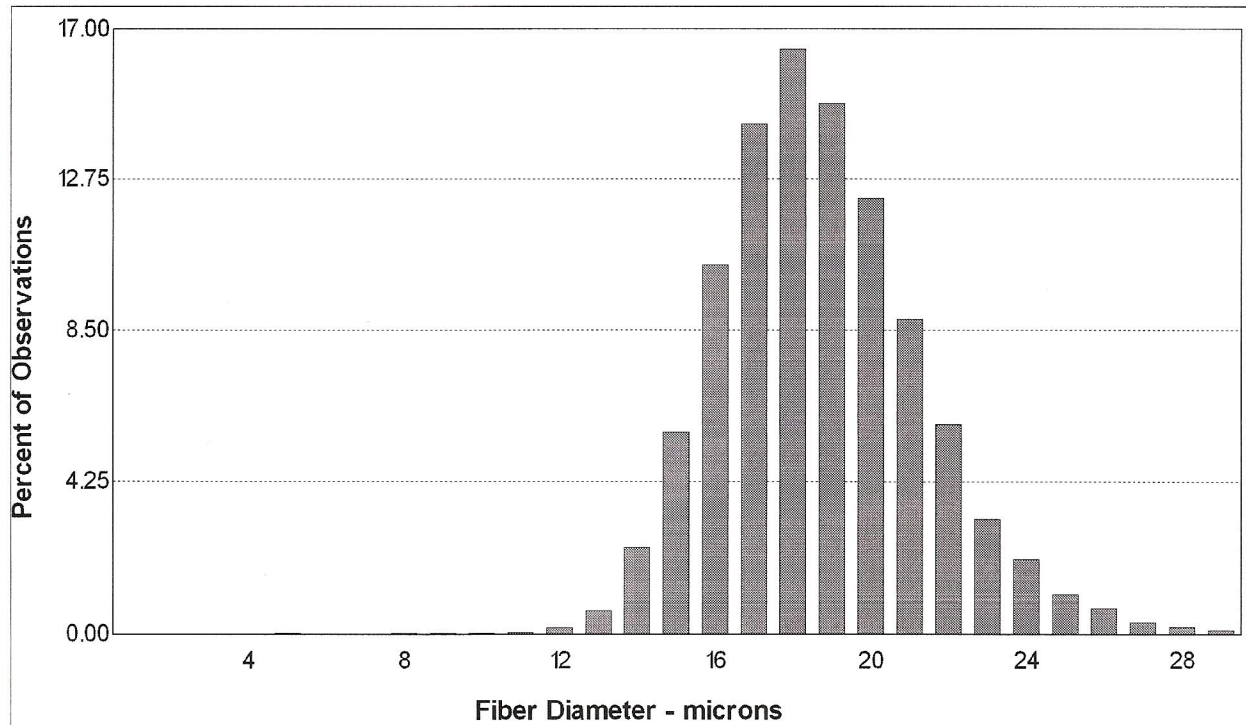

This Test Performed According to I.W.T.O Method 47