

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Holland/Jan van den Hoek  
Rijksstraatweg 94  
Numansdorp 3281LW Netherlands

Date: 06/04/1

Test No: 45505


### Animal and Sample Description

Animal Name: AH Peruvian Christiano  
Breed: Alpaca(Huacaya)  
Sex: Male  
Color: White

Animal ID: 0006E8ED4B  
Sample Location: Side  
Sample Date: 04/22/13  
Age: 06/21/09

### Laboratory Data

Mean Fiber Diameter:	20.8 microns	Fibers Greater Than 30 microns:	3.2 %
Standard Deviation:	4.3 microns	Comfort Factor:	96.8 %
Coefficient of Variation:	20.7 %	Mean Curvature:	41.1 deg/mm
Spin Fineness:	20.2 microns	SD Curvature:	22.7 deg/mm

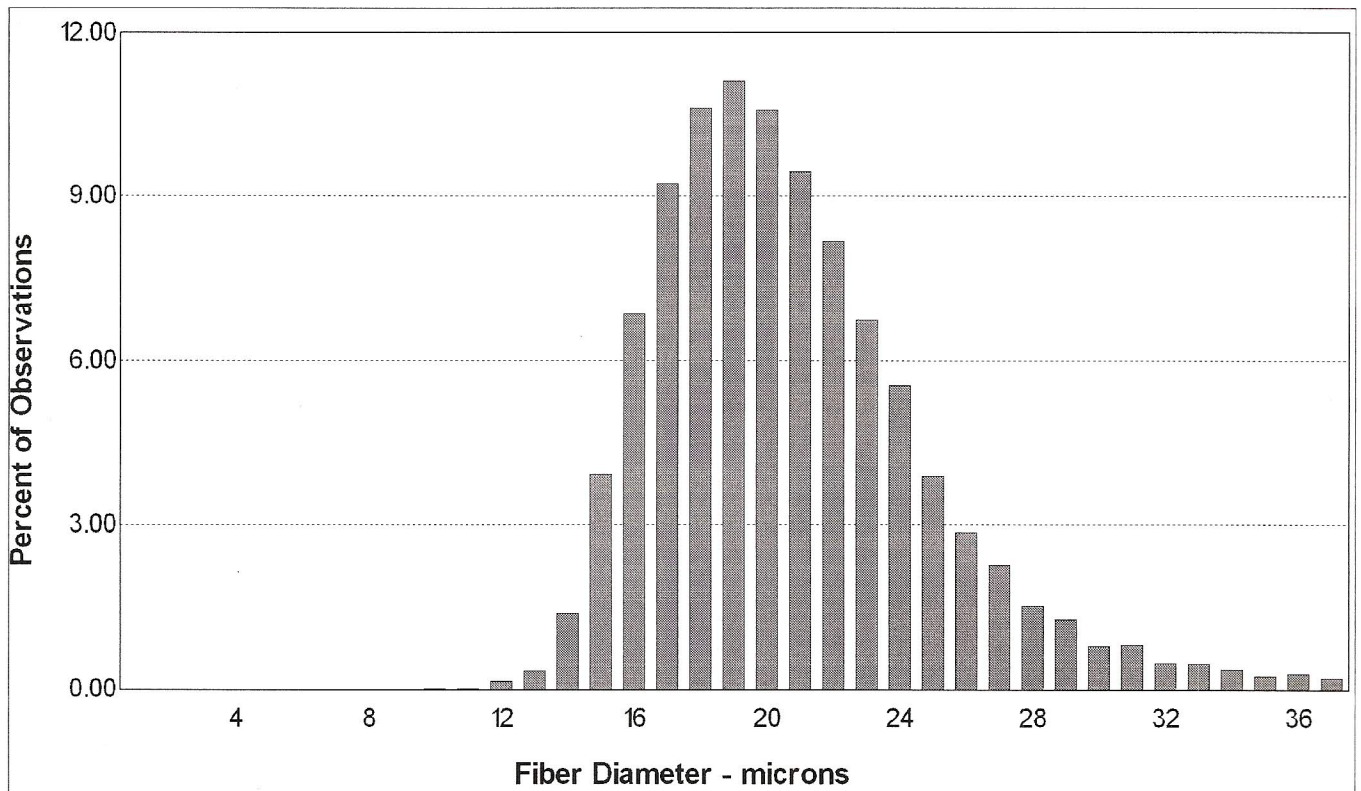

This Test Performed According to I.W.T.O Method 47