



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281LW Netherlands

Date: 06/04/1

Test No: 45506


Animal and Sample Description

Animal Name: AH Peruvia Vengador
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 0006E946F5
Sample Location: Side
Sample Date: 04/22/13
Age: 07/07/09

Laboratory Data

Mean Fiber Diameter:	23.4 microns	Fibers Greater Than 30 microns:	6.1 %
Standard Deviation:	4.4 microns	Comfort Factor:	93.9 %
Coefficient of Variation:	18.8 %	Mean Curvature:	40.7 deg/mm
Spin Fineness:	22.3 microns	SD Curvature:	22.9 deg/mm

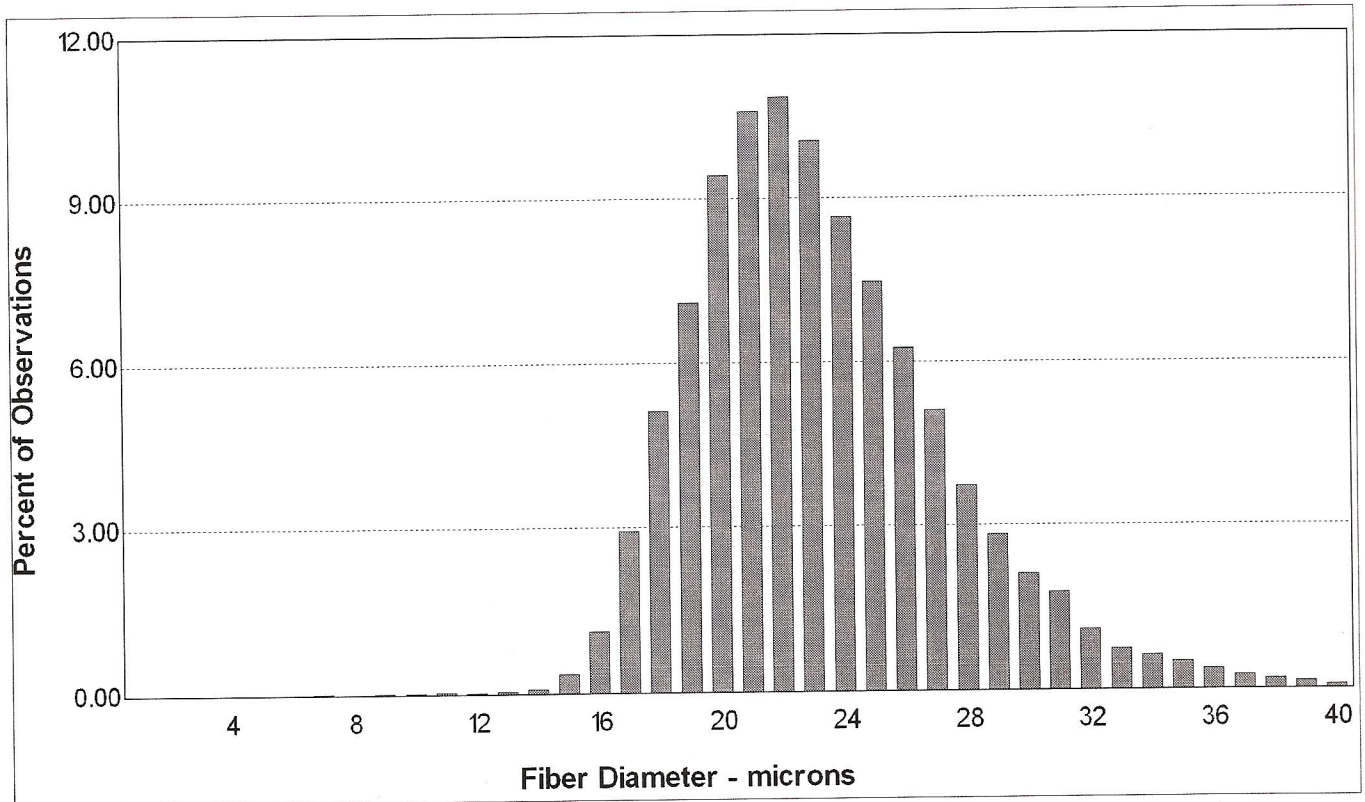

This Test Performed According to I.W.T.O Method 47