

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Alpaca Holland/Jan van den Hoek  
Rijksstraatweg 94  
Numansdorp 3281LW Netherlands

07/28/12

Test No: 436927


### Animal and Sample Description

**Animal Name:** Peruvian Armando of Wessex  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 982009105077814  
**Sample Location:** Side  
**Sample Date:** 05/02/12  
**Age:** 08/09/07

### Laboratory Data

<b>Mean Fiber Diameter:</b>	19.8 microns	<b>Spin Fineness:</b>	18.5 microns
<b>Standard Deviation:</b>	3.2 microns	<b>Mean Curvature (deg/mm):</b>	46.6
<b>Coefficient of Variation:</b>	15.9 %	<b>SD Curvature (deg/mm):</b>	25.1
<b>Fibers Greater Than 30 microns:</b>	0.4 %	<b>Comfort Factor:</b>	99.6 %
<b>Medullated Fibers:</b>	7.6 %		

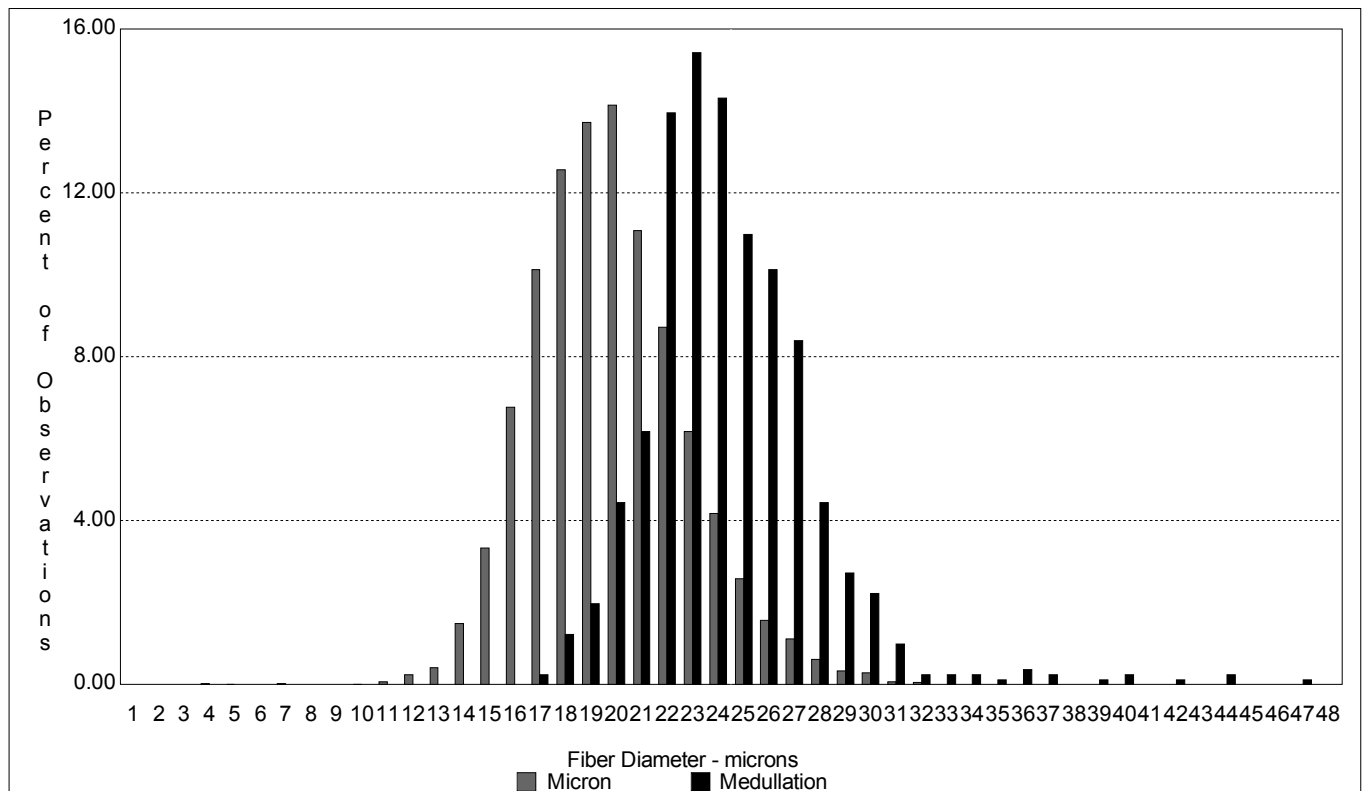

This Test Performed According to I.W.T.O Method 47